

Calibration Standards/Instruments and Accredited Calibration Services

Catalog No. E4163



**Accredited Calibration Services
for Implementing Traceability of
Measurements from a World Leader in
Dimensional Metrology.**

Mitutoyo

Traceability of the accuracy of measuring instruments put its basis on the calibration standards and instruments that are traceable to nationally or internationally recognized standards. Here is an introduction to our accredited calibration laboratories, traceability system and ISO 9000 based manufacturing/sales/service activities conducted worldwide followed by a quick reference to calibration standards and instruments available from Mitutoyo as appropriate for maintaining the accuracy of precision measuring tools and instruments.

Worldwide Accredited Calibration Laboratories	3
Traceability System to National Standard	5
Attaining ISO 9000 Registration	6
Conformance to CE Marking	7
Gauge Blocks ... the basic reference in metrology	8
Calibration standards/instruments available from Mitutoyo for the measuring instruments	

Gauge blocks

Automatic Gauge Block Interferometer GBI	10
Frequency Stabilized He-Ne Laser Light Source	10
Long Gauge Block Interferometer LGBI	11
Differential Type Automatic Gauge Block Comparator GBCD-100A	11
Differential Type Manual Gauge Block Comparator GBCD-250	12
Manual Gauge Block Comparator GBCS-250	12

Ring gauges

Ring Gage Measuring Machine, Ring Master RM-120	13
---	----

Outside micrometers

Gauge Block Set for Micrometer Inspection	14
Micrometer Standards	14
Optical Parallels	14
Optical Flats	14

Inside Micrometers

CERA-Inside Micro-Checker	15
---------------------------	----

Bore Gages

Height Master	19
---------------	----

Depth Micrometers

Depth Micro-Checker	15
---------------------	----

Calipers

CERA Caliper Checker	15
----------------------	----

Height Gages

CERA Caliper Checker	17
Height Master	19
Check Master	16

CMMs/Machine Tools

Granite Surface Plate (Graplate)	19
----------------------------------	----

Dial Indicators/Dial Test Indicators

Dial Gage Tester (170 Series)	17
Calibration Tester (521 Series)	17

Electronic Micrometers

Calibration Tester (521 Series)	17
---------------------------------	----

Coordinate Measuring Machines

Check Master	16
Quadra-Square Master	16

Profile Projectors/Measuring Microscopes

Standard Scales and Reading Scales (172 series)	18
Standard Scales (182 series)	18
Working Standard Scales (182 series)	18

Snap Gages (C-gages)

Snap Gage Checker	19
-------------------	----

Height Measurement Standard/Surface Plate

Height Master/Graplate	19
------------------------	----

Scope of end standard calibration

At Utsunomiya Calibration Center

Type	Comparison
Range	0.6mm up to 600mm (at comparison)
Measurement uncertainty (coverage factor K=2)	
0.5mm up to 100mm	0.06µm
Over 100mm up to 600mm	(0.03+L/2300)µm*

Laser wavelength

Range	633nm
Measurement uncertainty (coverage factor K=2)	(5.0X10 ⁻¹¹)

Standard scale

Range	Up to 500mm
Measurement uncertainty (coverage factor K=2)	
Up to 300mm	0.33µm
Over 300mm up to 500mm	(0.3+L/10000)µm

Temperature

Range	0°C up to 40°C
Type	Comparison
Masurement uncertainty (coverage factor K=2)	
Up to 300mm	0.33µm
Over 300mm up to 500mm	(0.3+L/10000)µm
Platinum Resistance Thermometer (Four wires system, 100Ω)	6mK
Platinum Resistance Thermometer (Three wires system, 1000Ω)	50mK
Thermometer with Indicator	8mK
*L=nominal length (µm)	

At Miyazaki Plant

Type	Interferometry and Comparison
Range	0.1mm up to 1000mm
Measurement uncertainty (coverage factor k=2)	
0.1mm up to 100mm	0.04µm
Over 100mm up to 600mm	(0.02+L/4000)µm*



Worldwide Accredited Calibration Laboratories

Being nationally accredited calibration laboratories, Mitutoyo conducts calibration services at various parts of the globe to help customers implement and maintain the traceability of accuracy of their precision measuring tools and instruments. Scope of calibration service at each of our 16 accredited calibration laboratories is shown below.

Calibration: A set of operations which establishes, under specified conditions, the relationship between values indicated by measuring instrument or system, or values represented by a material measure or a reference material, and the corresponding known values realized by standards. (VIM, 1993)


Department of accreditation	Registered	Scope Standard	Accreditation body of calibration service	Accreditation	Accredited No. date	
Miyazaki Plant	ISO/IEC 17025 ISO/IEC 17025	Gauge Block Gauge Block, Cera Straight Maser	NITE/IAJapan (JCSS) RvA	0030 K 107	1994-05-02 1997-02-20	
Kiyohara Calibration Center	ISO/IEC 17025	Line Standard (Standard Scale)	NITE/IAJapan (JCSS)	0067	1996-08-07	
Tsukuba Calibration Center	ISO/IEC 17025	Laser Platinum Resistance Thermometer, Thermometer with Indicator	NITE/IAJapan (JCSS)	0031	1994-05-02 2003-12-10	
Utsunomiya Calibration Center	ISO/IEC 17025	Gauge Block, Step Gage, Caliper...etc (11item)	NITE/IAJapan (JCSS)	0078	1998-05-06	
Kawasaki Calibration Center	ISO/IEC 17025	Caliper, Micrometer, Electronic Micrometer...etc (4item)	RvA	K 125	2001-01-24	
Hiroshima Calibration Center	ISO/IEC 17025	Step Gage, Caliper...etc (8item)	NITE/IAJapan (JCSS)	0109	2002-04-11	
Techno Service Business Division	ISO/IEC 17025	CMM, Profile projectors, Measuring microscopes	RvA	K 132	2003-12-17	
Akashi Calibration Center	ISO/IEC 17025	Force-Proving Instrument : Compressive Force	NITE/IAJapan (JCSS)	0086	2000-05-30	
Mitutoyo (UK)	ISO/IEC 17025	Gauge Block, Caliper, CMM...etc (40item)	UKAS	0332	1991-07-30	
MAS	Length	ISO/IEC 17025	Gauge Block, Caliper, CMM...etc (19item)	RBC	031	1992-09-15
	Hardness	ISO/IEC 17025	Rockwell Tester	RBC	207	2002-09-20
Argentine	ISO/IEC 17025	Rockwell Tester	OAA	LC 010	2002-11-07	
Mitutoyo (NL)	ISO/IEC 17025	Gauge Block, Caliper, CMM...etc (12item)	RvA	K 086	1994-10-14	
Mitutoyo (D)	ISO/IEC 17025	Gauge Block, Caliper...etc (10item)	DKD	DKD-K-14501	1995-01-10	
MAP	Singapore	ISO/IEC 17025	Gauge Block, Caliper, CMM...etc (15item)	SAC-SINGLAS	LA-1996-0102-C	1996-11-08
	Indonesia	ISO/IEC 17025	Surface roughness instruments, CMM...etc (7item)	SAC-SINGLAS	LA-1996-0102-C-1	2003-06-14
Mitutoyo (Switzerland)	ISO/IEC 17025	Gauge Block, Caliper, CMM...etc (9item)	SAS	SCS 074	1996-12-1	
MAC	Elk Grove Lab.	ISO/IEC 17025	Gauge Block, Caliper, CMM...etc (27item)	A2LA	0750.01	1998-04-20
	Plymouth Lab.	ISO/IEC 17025	Gauge Block, Caliper, Electronic Micrometer...etc (10item)	A2LA	1472.01	2000-02-03
	Aurora (field)	ISO/IEC 17025	CMM, Vision Measuring Machine...etc (5item)	A2LA	1643.01	2002-01-15
Mitutoyo (I)	ISO/IEC 17025	Gauge Block, Roundness standards, CMM...etc (4item)	SIT	107	1998-05-01	
Mitutoyo (Taiwan)	ISO/IEC 17025	Surface finish specimen, Toolmaker Microscope, CMM...etc (5item)	CNLA	0336	1998-06-15	
Mitutoyo (Malaysia)	ISO/IEC 17025	Caliper, Surface roughness instruments, CMM...etc (13item)	SAMM	SAMM-152	1998-10-15	
Mitutoyo (Mex)	Length	ISO/IEC 17025	Gauge Block, Caliper, CMM...etc (20item)	EMA	D-45	2000-11-21
	Hardness	ISO/IEC 17025	Rockwell Tester	EMA	DZA-10	2003-02-18
Mitutoyo (Scandinavia)	ISO/IEC 17025	Gauge Block, CMM	SWEDAC	1794	2002-03-04	

NITE: National Institute of Technology and Evaluation
 JCSS: Japan Calibration Service System
 RvA NKO: Nederlandse Kalibratie Organisatie
 UKAS: United Kingdom Accreditation Service
 RBC: Rede Brasileira de Calibração
 DKD: Deutscher Kalibrierdienst
 SAC: Singapore Accreditation Council
 SACSINGLAS: Singapore Accreditation Council-Singapore
 Laboratory
 SINGLAS: Accreditation Scheme

SAS: Swiss Accreditation Service
 A2LA: American Association for Laboratory Accreditation
 SIT: Servizio di Taratura in Italia
 CNLA: Chinese National Laboratory Accreditation
 DSM: Department of Standards Malaysia
 SAMM: Skim Akreditasi Makmal Malaysia
 TISI: Thai Industrial Standard Institute
 EMA: Entidad Mexicana de Acreditación, a.c.
 SINGLAS: Accreditation Scheme
 SWEDAC: Swedish Board for Accreditation and Conformity
 Assessment

Traceability System to National Standard


Mitutoyo Group Accredited Calibration Laboratories

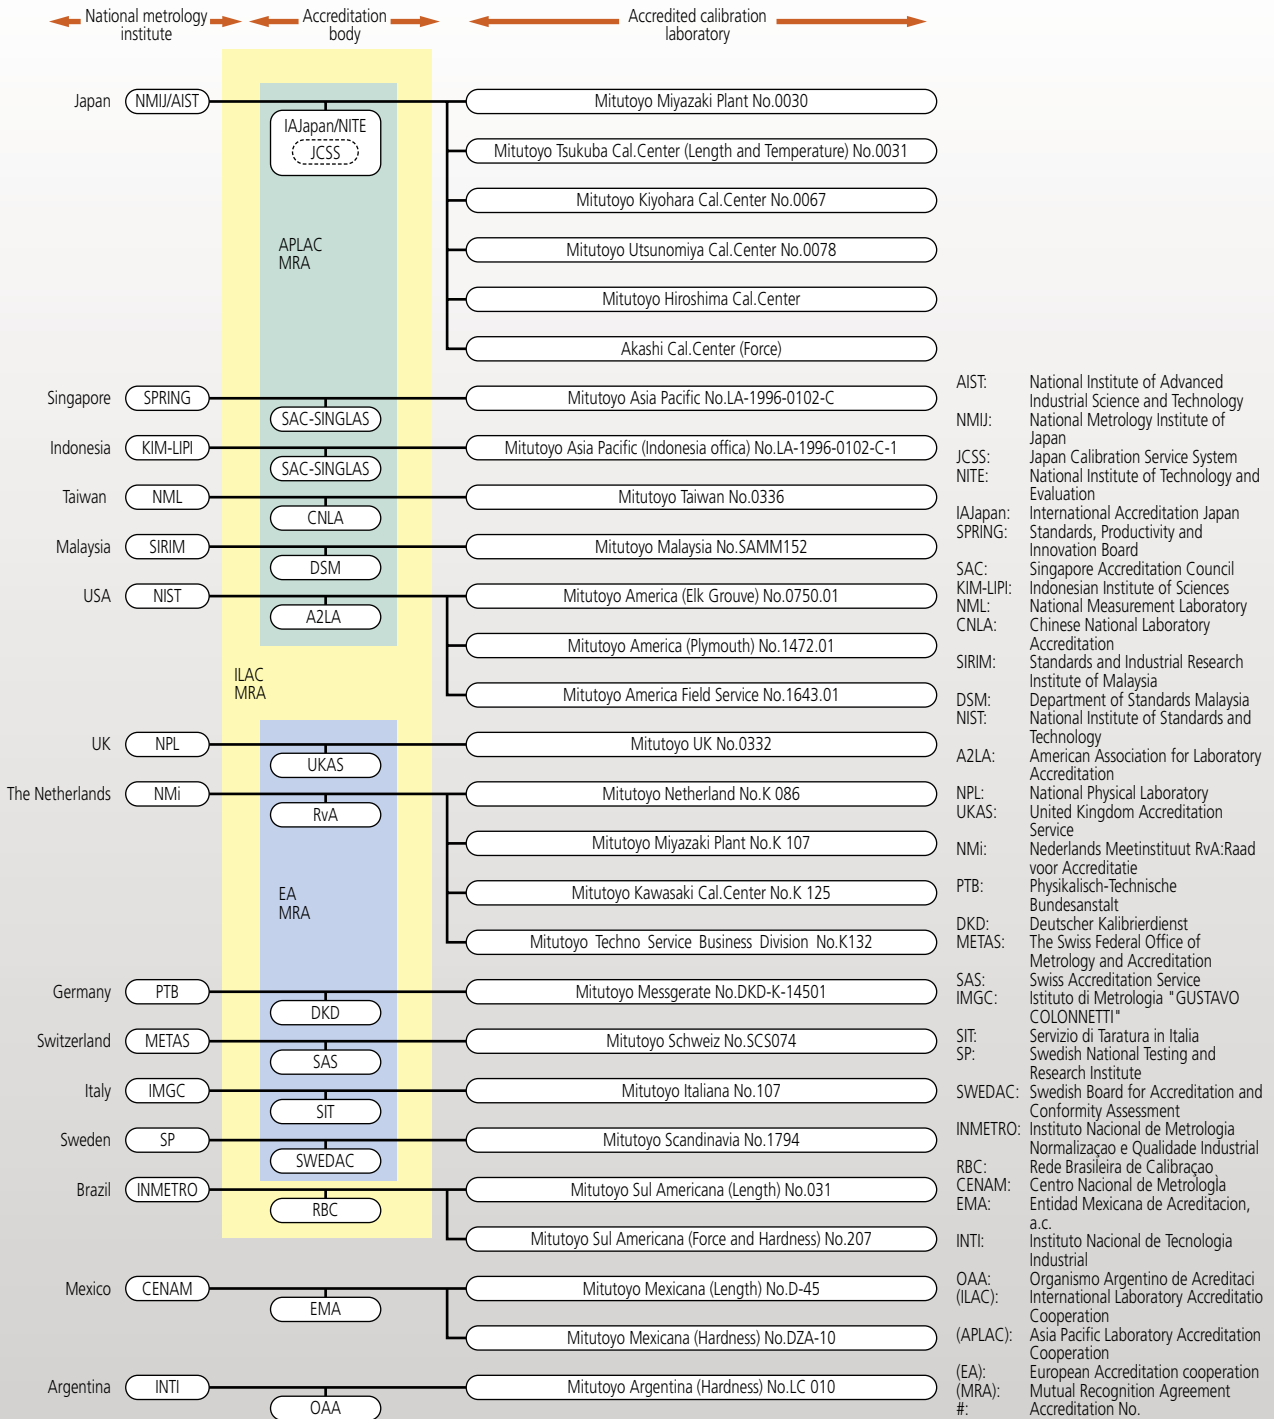

Traceability system of length standard

Traceability: Property of the result of a measurement or the value of a standard whereby it can be related to stated reference, usually national or international standards, through an unbroken chain of comparisons all having stated uncertainties.

Traceability of the accuracy of measuring instruments: A documented chain of comparison connecting the accuracy of a measuring instrument to other measuring instruments of higher accuracy and ultimately to a primary standard.

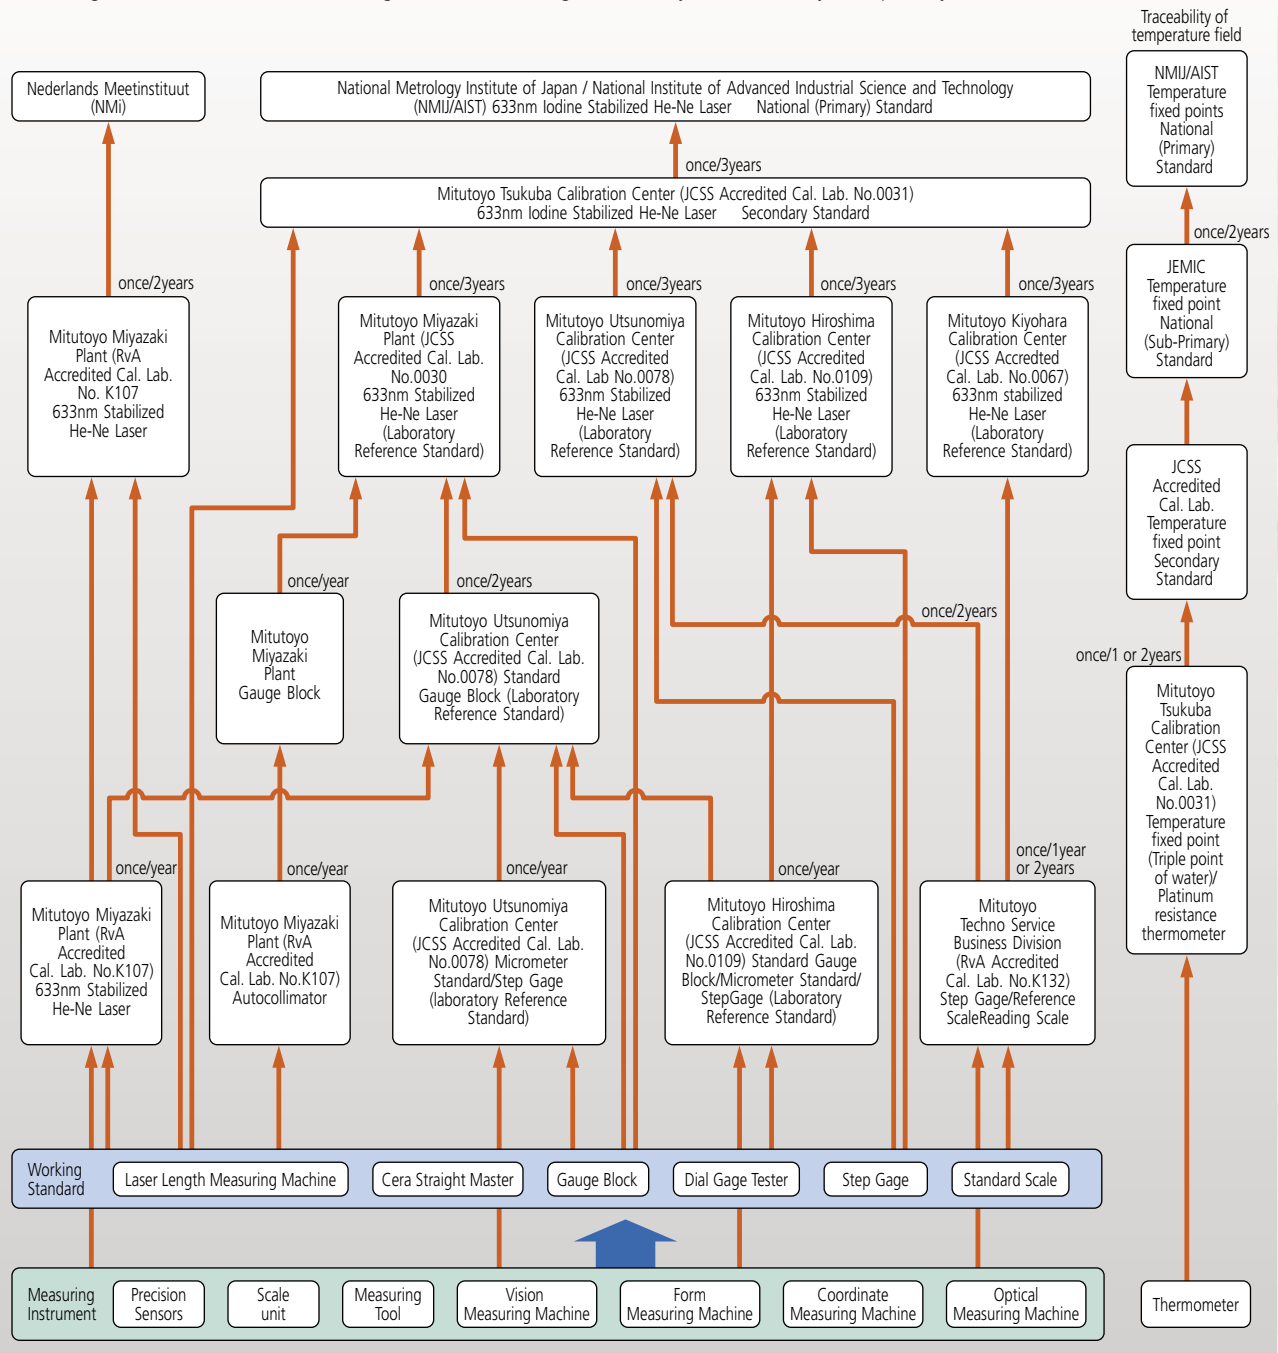


Attaining ISO 9000 Registration

As a world leading manufacturer of precision measuring instruments, Mitutoyo has implemented ISO 9000 certified quality systems at various sites within the organization all over the globe to better serve customers in dimensional metrology, the basic technology in quality management and quality assurance for all of the manufacturing industries.

Registered Supplier	Registered Standard	Products or Services	Registration Bodies	Registration Number
Miyazaki Plant	ISO9001:2000	Manufacture and recalibration of gauge blocks, setting rings, micrometer standard bars.	JMI(JQA)	JMI-0189
Kiyohara Plant	ISO9001:2000	Design/development and manufacture of linear scale	JMI(JQA)	JMI-0241
Tool&Gauge Plant	ISO9001:2000	Design/development, manufacture and servicing (repair of field returns) of vernier, dial and digital caliper excluding calipers with special measuring faces (jaws), height gauges, depth gauges, digimatic scale unit and linear height.	JQA	JQA-0304
Shiwa Plant	ISO9001:2000	Design/development, manufacture and servicing (supply of repair part) of micrometers.	JQA	JQA-0319
Microcord Plant	ISO9001:2000	Design/development and manufacture and servicing of coordinate measuring machine and precision granite surface plate	JQA	JQA-0542
Kure Plant	ISO9001:2000	Development, design, production and servicing of surface roughness measuring machines, contour measuring machines, roundness measuring machines, optical instruments (profile projectors, measuring microscopes), vision measuring machines and working standards	JSA-Q	JSAQ052
Techno Service Business Division	ISO9001:2000	Installation, maintenance, inspection and calibration of coordinate measuring machines, form measuring instruments, optical instruments and small measuring tools.	JSA-Q	JSAQ054
Nakatsugawa Plant	ISO9001:2000	<ul style="list-style-type: none"> •Design/development and manufacture of dial indicators, lever type dial indicators and digital dial indicators (digimatic indicators). •The repair of field returns of digital indicators (digimatic indicators). 	JQA	JQA-QM3695
Gohara Material Plant	ISO9001:2000	Manufacturing of cast iron, cast steel, nonferrous alloy, raw materials and ceramic slip cast and parts for measuring tools, and instruments, those machining and painting.	JQA	JQA-QM7729
Akashi Corporation Sagami Plant	ISO9001:2000	Sales, design/development and manufacture of hardness testing machines, vibrometers, seismological instruments, vibration testing machines, balancing machines. In-house repair of hardness testing machines.	JQA	JQA-0323
Mitutoyo Sul Americana Ltda	ISO 9001:2000	Suzano Plant Development, manufacture and sales of coordinate measuring machines, calipers, micrometers etc.	ABS QE	30697
Mitutoyo Messgeräte GmbH	ISO 9001:2000	Distribution and service of measuring instruments and complex measuring systems for production measuring technology	TÜV	01100026017
Mitutoyo Italiana S.R.L.	ISO 9001:2000	Sales and distribution of MITUTOYO precision measuring equipment. Customer support services including technical support, repair, associated calibration and training for measuring equipment.	LRQA	170323
Mitutoyo France S.A.R.L.	ISO 9001:2000	Sales, distribution and after sales service of precision measurement for metrology equipments including installation, maintenance, repair and internal calibration.	AB Certification	A346
Mitutoyo Scandinavia AB	ISO 9001:2000	Sales, service and calibration of precision measuring equipment.	DNV	2000-SKM-AQ-1578
Mitutoyo Nederland B.V.	ISO 9001:2000	Veenendaal Plant The production of manual and NC coordinate measuring machines.	LRQA	654274
Mitutoyo Measuring Instruments (Suzhou) Co.,Ltd	ISO9001:2000	Manufacture of digital caliper and black granite surface plate	CQC	32000/200110113

The ISO 9000 series comprises three major standards ISO 9001, 9002, and 9003, each of which certifies a different range and scope of operations as shown below.

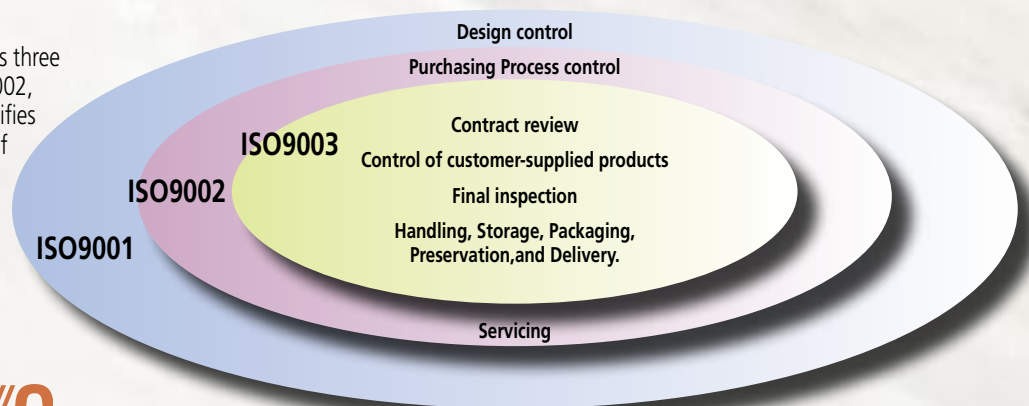

Conformance to CE Marking

Safety is one of our major concerns associated with quality assurance in serving customers. Conformance to CE marking is a means of our safety improvement activities and so established and implemented are programs at each plant to comply with the Machinery Directives, the EMC Directives, and the Low Voltage Directives as appropriate. We have set up facilities for CE marking compliance evaluation. Products being shipped with the CE mark conforms to the requirements set forth by the European Community for safety, health, environment and customer protection. (CE stands for "Conformite Europeenne".)



Compliance evaluation of CE marking in Mitutoyo facility (EMC Directives)



EC Directives concerned

NEC Directives	Scope	Date effective
Machinery Directive	Products that may result in personal injury due to moving parts of the machine, including motors, etc.	January 1st, 1995
EMC Directive (Electromagnetic Compatibility)	Tools (instruments) that are subject to electromagnetic interference or tools (instruments) of which the performance is subject to such interference.	January 1st, 1996
Low Voltage Directive	Tools (instruments) in which there is a risk of receiving an electric shock, burn, radioactivity, etc., and that operate on either of the following voltages: AC voltage: 50 to 1000V DC voltage: 75 to 15000V	January 1st, 1997

Gauge Blocks ...the basic reference in metrology...

The most popular end standard in industrial dimensional measurement is available in both the rectangular gauge block and square gauge block in type and in steel or ceramic in material.

Rectangular Gauge Block

Steel and ceramic-type gauge blocks are offered.

- For more information about individual block lengths, refer to Catalog No. E4092 "Gauge Blocks".



103-piece set (steel)



103-piece set (ceramic)



Long gauge block set

Order No. (DIN/JIS block set only)

Type	Blocks per set	Accuracy	Steel	Ceramic
1mm base sets	112	Grade K	516-937-60	516-337-60
		Grade 0	516-938-10	516-338-10
		Grade 1	516-939-10	516-339-10
		Grade 2	516-940-10	516-340-10
	103	Grade K	516-941-60	516-341-60
		Grade 0	516-942-10	516-342-10
		Grade 1	516-943-10	516-343-10
		Grade 2	516-944-10	516-344-10
	88	Grade 0	516-970-10	—
		Grade 1	516-971-10	—
		Grade 2	516-972-10	—
	87	Grade K	516-945-60	516-345-60
Grade 0		516-946-10	516-346-10	
Grade 1		516-947-10	516-347-10	
Grade 2		516-948-10	516-348-10	
76	Grade K	516-949-60	516-349-60	
	Grade 0	516-950-10	516-350-10	
	Grade 1	516-951-10	516-351-10	
	Grade 2	516-952-10	516-352-10	
56	Grade K	516-953-60	516-353-60	
	Grade 0	516-954-10	516-354-10	
	Grade 1	516-955-10	516-355-10	
	Grade 2	516-956-10	516-356-10	
47	Grade K	516-957-60	516-357-60	
	Grade 0	516-958-10	516-358-10	
	Grade 1	516-959-10	516-359-10	
	Grade 2	516-960-10	516-360-10	
47	Grade K	516-961-60	516-361-60	
	Grade 0	516-962-10	516-362-10	
	Grade 1	516-963-10	516-363-10	
	Grade 2	516-964-10	516-364-10	
46	Grade K	516-994-60	516-394-60	
	Grade 0	516-995-10	516-395-10	
	Grade 1	516-996-10	516-396-10	
	Grade 2	516-997-10	516-397-10	
32	Grade K	516-965-60	516-365-60	
	Grade 0	516-966-10	516-366-10	
	Grade 1	516-967-10	516-367-10	
	Grade 2	516-968-10	516-368-10	

Type	Blocks per set	Accuracy	Steel	Ceramic
2mm base sets	112	Grade K	516-513-60	—
		Grade 0	516-514-10	—
		Grade 1	516-515-10	—
		Grade 2	516-516-10	—
	88	Grade K	516-501-60	—
		Grade 0	516-502-10	—
		Grade 1	516-503-10	—
		Grade 2	516-504-10	—
	88	Grade K	516-517-60	—
		Grade 0	516-518-10	—
		Grade 1	516-519-10	—
		Grade 2	516-520-10	—
47	Grade K	516-521-60	—	
	Grade 0	516-522-10	—	
	Grade 1	516-523-10	—	
	Grade 2	516-524-10	—	
46	Grade K	516-505-60	—	
	Grade 0	516-506-10	—	
	Grade 1	516-507-10	—	
	Grade 2	516-508-10	—	
33	Grade K	516-509-60	—	
	Grade 0	516-510-10	—	
	Grade 1	516-511-10	—	
	Grade 2	516-512-10	—	
0.001mm step block sets	18	Grade K	516-973-60	516-373-60
		Grade 0	516-974-10	516-374-10
		Grade 1	516-975-10	516-375-10
		Grade 2	516-976-10	516-376-10
9	Grade K	516-981-60	516-381-60	
	Grade 0	516-982-10	516-382-10	
	Grade 1	516-983-10	516-383-10	
	Grade 2	516-984-10	516-384-10	
9	Grade K	516-985-60	516-385-60	
	Grade 0	516-986-10	516-386-10	
	Grade 1	516-987-10	516-387-10	
	Grade 2	516-988-10	516-388-10	
Thin block sets	9	Grade 0	516-990-10	—
		Grade 1	516-991-10	—
		Grade 2	516-992-10	—
Long Block set	8	Grade K	516-701-60	516-731-60
		Grade 0	516-702-10	516-732-10
		Grade 1	516-703-10	516-733-10
		Grade 2	516-704-10	516-734-10
Wear block sets*	2	Grade 0	516-807-10	516-832-10
		Grade 1	516-806-10	516-833-10
2	Grade 0	516-803-10	516-830-10	
	Grade 1	516-802-10	516-831-10	

Grade K gauge blocks are complete with the Certificate of Inspection and Certificate of Calibration.

* Wear blocks are made of tungsten carbide.

Square Gauge Block

The gauge blocks have a square measurement surface of 24.1 x 24.1mm and a ϕ 6.7mm through hole at the center to improve ease-of-use and for use in a wide range applications.

- These gauge blocks can be wrung to one another and can be used for making tools and dedicated gages.
- Gauge blocks can be joined using the optional tie rod, screws, and nuts.
- For more information, refer to Catalog No. E4092 "Gauge Blocks".



112-piece set

Order No. (DIN/JIS block set only)

Blocks per set	Accuracy	Steel	Ceramic
112	Grade 0	516-438-10	—
	Grade 1	516-439-10	—
	Grade 2	516-440-10	—
103	Grade 0	516-442-10	—
	Grade 1	516-443-10	—
	Grade 2	516-444-10	—
76	Grade 0	516-450-10	—
	Grade 1	516-451-10	—
	Grade 2	516-452-10	—
47	Grade 0	516-458-10	—
	Grade 1	516-459-10	—
	Grade 2	516-460-10	—
32	Grade 0	516-466-10	—
	Grade 1	516-467-10	—
	Grade 2	516-468-10	—
8*	Grade 0	516-752-10	—
	Grade 1	516-753-10	—
	Grade 2	516-754-10	—
2**	Grade 0	516-820-10	—
	Grade 1	516-821-10	—
2**	Grade 0	516-822-10	—
	Grade 1	516-823-10	—

Provided with Certificate of Inspection.

*Long gauge block set.

**Wear gauge block sets made of carbide.

Individual Gauge Block

- If frequently measuring a specific length, it is a good idea to purchase an individual gauge block.
- For more information about individual block lengths, refer to Catalog No. E4092 "Gauge Blocks".



Gauge Block Accessory Sets

To expand the variety of rectangular gauge block applications, Mitutoyo offers the Gauge Block Accessories Set. By assembling the items in the set, you can build up various precision measuring setups with gauge blocks easily and quickly.

For more information, refer to Catalog No. E4092 "Gauge Blocks".



516-601
Rectangular gauge block
accessory set



516-611
Square gauge block
accessory set

Order No.

Order No.	Description
516-601	22-piece set for rectangular gauge block
516-602	14-piece set for rectangular gauge block
516-605	For long rectangular gauge block (over 125mm)
516-611	For square gauge block

Micro Checker

- Can be measured in both vertical and horizontal posture.
- Parallelism is measured by attaching the Optical parallel (optional accessory) to the GB set.

Order No.	516-607 (mm type)	516-608 (inch type)
Applicable Gauge Block	516-106, 516-107, 516-108, 516-156, 516-157, 516-158	516-921, 516-922, 516-923, 516-321, 516-322, 516-323
Applicable Gauge Block size	2.5, 5.1, 7.7, 10.3, 12.9, 15, 17.6, 20.2, 22.8, 25mm	.105, .210, .315, .420, .5, .605, .710, .815, .920inch
Mass	N/W1300g	G/W1300g/2.87lbs. (with wooden box)



Gauge Block Calibration

Automatic Gauge Block Interferometer GBI

Target preliminary measurement range expanded sevenfold with two wavelengths

The Two-Wavelength Automatic Gauge Block Interferometer, GBI is an easy to use gauge block interferometer capable of absolute measurement of central length of gauge blocks with the utmost accuracy.

- Two He-Ne laser light sources are adapted to ensure extremely reliable measurements. Preliminary measurement with up to 1 μ m uncertainty is satisfactory for interferometry with the GBI.
- No human intervention in observing the interference fringes. This eliminates human errors in measurements.
- Remote control of the system is possible in measurement. This facilitates preventing the operator heat from affecting the gauge blocks inside the interferometer.
- Air refractive index correction and gauge block thermal expansion correction are automatically performed with the computer connected to the thermometer, hygrometer, and barometer.
- An array of 12 gauge blocks set up within the interferometer can be continuously measured within 5 minutes for each block.



Specifications

Light source	He-Ne laser (633nm and 543nm)
Measuring range	Up to 250mm
Uncertainty of measurement: (Coverage factor k=2)	$0.025\mu\text{m} + 0.2 \times 10^{-6}L$ L=nominal length (μm)
Number of blocks installable	12 pcs.

Frequency Stabilized He-Ne Laser Light Source LIS-633B, LIS-543

Frequency stabilized He-Ne laser is available as a light source for such applications as length measurement, interferometry, spectrograph, and holography.

- Frequency stabilized high intensity single mode linear polarized He-Ne laser.

Specifications

Model	LIS-633B	LIS-543
Wavelength	633nm	543nm
Wavelength stabilit	1×10^{-9} /year	2×10^{-9} /year
Output	1mW or over	150 μ W or over
Beam diameter	0.6mm	0.6mm
Class	Class 3B	Class 3A
Ambient temperature	20°C \pm 5°C	20°C \pm 5°C
Dimensions (WxHxD)	134x121x396 mm	134x121x396 mm




Gauge Block Calibration

Long Gauge Block Interferometer LGBI

Target preliminary measurement range expanded sevenfold with two wavelengths

This interferometer determines the deviation of the central length of long rectangular gauge blocks of 100mm to 1016mm with high accuracy. A maximum of 4 gauge blocks can be set up at a time, permitting measurements to be performed efficiently with the reduced time for thermal stabilization of the gauge blocks.

- Two He-Ne laser light sources are adopted to ensure extremely reliable measurements. Preliminary measurement with up to 1 μ m uncertainty is satisfactory for interferometry with the LGBI.
- Observation of interference fringe is possible either via CCD camera (optional) or eyepiece lens.
- The interferometer chamber can accommodate up to 4 gauge blocks.
- Gauge blocks can be set up horizontally at Airy points (0.211L from each end).
- Air refractive index correction is possible by directly measuring the index in the vacuum cell or by measuring temperature, humidity and barometric pressure.

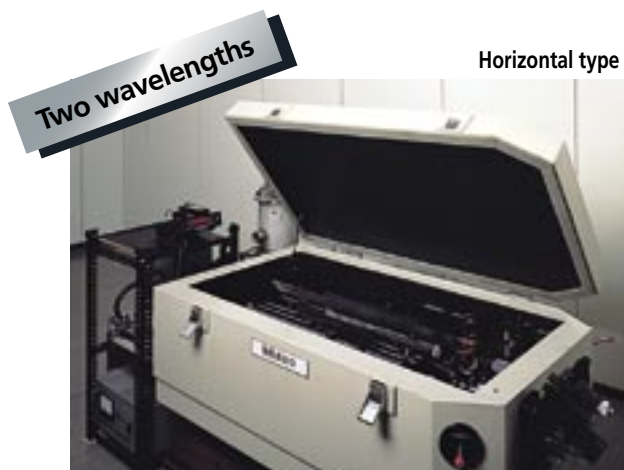

Specifications



Light source	He-Ne laser (633nm and 543nm)
Measuring range	100mm to 1016mm
Calibration function	Absolute optical path length difference measurement with gauge block wrung to the platen
Uncertainty of measurement: (Coverage factor k=2)	0.03 μ m+0.2x10 ⁻⁶ L L=nominal length (μ m)

Differential Type Automatic Gauge Block Comparator GBCD-100A

ISO recommended differential type with dual gage head for automatic high accuracy measurement

Dual head type of gauge block comparator capable of automatic calibration of gauge block lengths between 0.5mm and 100mm with reference to the reference gauge block.

- Dual head feature eliminates the error due to the warp of thin gauge block.
- Automatically measures the center and four corners of a gauge block with reference to the central length of the reference gauge block.
- Calibration results are automatically processed with the GBPAK Calibration Program.
- Measurements for evaluation with ISO, JIS, DIN, ANSI, etc.

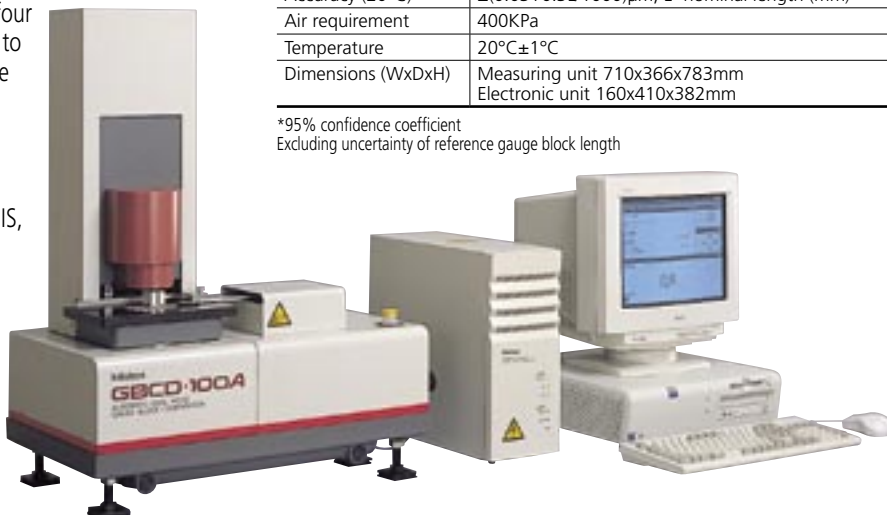

Specifications


Applications	Rectangular gauge blocks and square gauge blocks
Measuring range	0.5mm to 100mm
Display resolution	0.01 μ m
Measurement method	Differential measurement with dual head
Upper gaging head	Electric micrometer of 1N measuring force Carbide contact point of radius of 20mm
Lower gaging head	Electric micrometer of 0.6N measuring force Carbide contact point of radius of 5mm
Accuracy (20°C)*	$\pm(0.03+0.3L/1000)\mu$ m, L=nominal length (mm)
Air requirement	400KPa
Temperature	20°C \pm 1°C
Dimensions (WxDxH)	Measuring unit 710x366x783mm Electronic unit 160x410x382mm

*95% confidence coefficient
Excluding uncertainty of reference gauge block length

Gauge Block Calibration

Differential Type Manual Gauge Block Comparator GBCD-250

ISO recommended differential type with dual gage head. Long range Laser Hologage ($\pm 3\text{mm}$) allows 103 pieces gauge block set to be calibrated with a minimum number of reference gages.

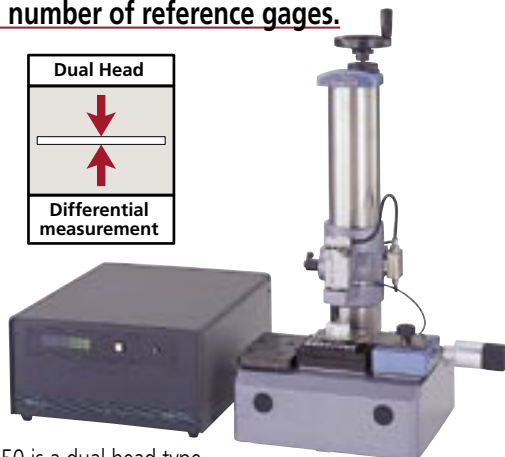

The GBCD-250 is a dual head type manual gauge block comparator capable of calibrating a wide range of gauge block lengths between 0.1mm and 250mm with a resolution to $0.01\mu\text{m}$ with the Mitutoyo Laser Hologage.

- Dual head feature eliminates the error due to warp of thin gauge blocks.
- A 103 gauge block set of grade 1 or 2 can be calibrated with only 8 reference gauge blocks thanks to the $\pm 3\text{mm}$ measuring range of the Laser Hologage.
- The Laser Hologage needs height positioning only to within $\pm 1\text{mm}$ otherwise required to within a few microns (μm), greatly reducing setup time.


Specifications

Applications	Rectangular gauge blocks and square gauge blocks
Measuring range	0.1mm to 250mm
Resolution	$0.01\mu\text{m}$
Measurement method	Differential measurement with dual head
Upper gaging head	Laser Hologage ($0.01\mu\text{m}$, $\pm 3\text{mm}$) of 0.8N measuring force Carbide contact point of radius of 20mm
Lower gaging head	Electric micrometer of 0.6N measuring force Carbide contact point of radius of 5mm
Accuracy (20°C)*	$\pm(0.03+0.3L/1000)\mu\text{m}$, L=nominal length (mm) (the nominal length must be the same for both the reference gauge block and the one to be calibrated) $\pm(0.06+0.3L/1000)\mu\text{m}$, L=nominal length (mm) (for grades 1 and 2: with the reference gauge block of length difference within $\pm 3\text{mm}$)
Temperature	$20^\circ\text{C}\pm 1^\circ\text{C}$
Dimensions (WxDxH)	Measuring unit 455x318x691mm Electronic unit 345x397x187mm (Excluding connectors)

* 95% confidence coefficient
Excluding uncertainty of reference gauge block length
GBPAC Calibration Program and personal computer are optional.

Manual Gauge Block Comparator GBCS-250

Long range Laser Hologage ($\pm 5\text{mm}$) allows 103 pieces gauge block set to be calibrated with a minimum number of reference gages.

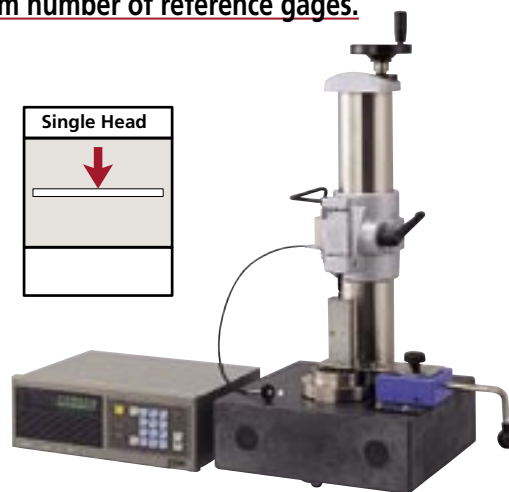

Single head type gauge block comparator capable of calibration of gauge blocks of length of 0.1mm up to 250mm with reference to the reference gauge blocks.

- Integrated with the Mitutoyo Laser Hologage ($\pm 5\text{mm}$ range), the GBCS-250 can calibrate a 103 gauge block set by using only 6 (for grade 2) or 8 (for grade 1) reference gauge blocks with the length difference of $\pm 5\text{mm}$. The Laser Hologage height positioning is required only to within 1mm against the reference gauge block otherwise required to within a few microns (μm), greatly reducing setup time.

Specifications

Applications	Rectangular gauge blocks and square gauge blocks
Measuring range	0.1mm to 250mm
Resolution	$0.01\mu\text{m}$
Measurement method	Single head
Gage head	Laser Hologage ($0.01\mu\text{m}$, $\pm 5\text{mm}$) of 0.8N measuring force Carbide contact point of radius of 20mm Anvil has a curvature
Accuracy (20°C)*	$\pm(0.03+0.3L/1000)\mu\text{m}$, L=nominal length (mm) (the nominal length must be the same for both the reference gauge block and the one to be calibrated) $\pm(0.06+0.3L/1000)\mu\text{m}$, L=nominal length (mm) (for grades 1 and 2: with the reference gauge block of length difference within $\pm 3\text{mm}$) $\pm(0.1+0.3L/1000)\mu\text{m}$, L=nominal length (mm) (for grades 2: with the reference gauge block of length difference within $\pm 5\text{mm}$)
Temperature	$20^\circ\text{C}\pm 1^\circ\text{C}$
Dimensions (WxDxH)	Measuring unit 300x300x686,5mm Electronic unit 235x115x118mm (Excluding connectors)

* 95% confidence coefficient
Excluding uncertainty of reference gauge block length
GBPAC Calibration Program and personal computer are optional.

Ring Gage Calibration

Ring Gage Measuring Machine Ring Master RM-120

Incorporated 120mm Laser Hologscale eliminates the need for multiple reference gages, permitting expertise-free high accuracy direct ring gage measurements with reduced total cost.

Incorporated with a high precision laser hologscale with a resolution of $0.01\mu\text{m}$, the Ring Master RM-120 directly measures the ring gage diameter between 6mm and 120mm without referring to otherwise required reference ring gages, efficiently and accurately. The measurement efficiency can be increased 100% over the conventional method where wringing gauge blocks is required.


- The laser hologscale eliminates the need for a reference gauge block set and reference ring gages.
- The line of measurement of the ring gage is on the axis of standard, meeting the Abbe's principle and ensuring higher measuring accuracy.
- Stylus change is not required for the entire measuring range.
- Enhanced repeatability and lower measuring force achieved with the air bearing on the stylus carriage guide.
- Workpiece alignment is easy to perform with the specially designed table which is capable of translation, tilting, elevation, and 90 deg rotation. The model with analog meter will further facilitate workpiece translation and tilting.



Standard counter type

Specifications

Measuring range	ID: 6mm to 120mm
Workpiece size	OD: 20mm to 200mm Thickness: up to 40mm
Measurement	Differential measurement with two styli
Display resolution	$0.1\mu\text{m}$
Accuracy ($\pm 2\sigma$) (20°C)*	$\pm(0.3+5D/1000)\mu\text{m}$, D=diameter to check (mm)
Repeatability ($\pm 2\sigma$)	$\pm 0.2\mu\text{m}$
Measuring force	Approx. 0.2N
Workpiece alignment	Centering range in XY plane: $\varnothing 2\text{mm}$ Tilting range about XY axis: $\pm 1/100$
Table elevation range	40mm during measurement Can down 50mm for workpiece loading/unloading
Air requirement	400kPa
Air consumption	Approx. 30L/min
Temperature	$20^\circ\text{C} \pm 0.5^\circ\text{C}$
Dimensions (WxDxH)	Standard counter type: 720x494x875mm Counter with analog meter type: 720x500x880mm

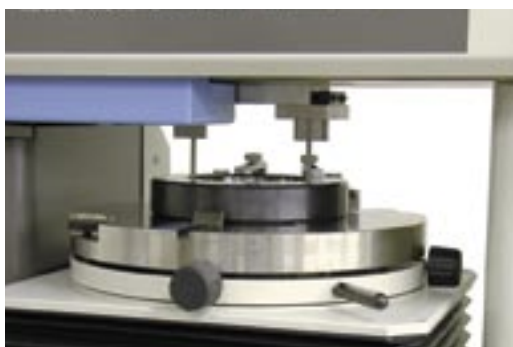

Outside Micrometer Calibration

Micrometer Inspection Gauge Block Set

Either set of gauge blocks can be used for measurement of outside micrometer errors, measurement surface flatness, and parallelism. For more information, refer to Catalog No. E4092 "Gauge Blocks".

10-piece ceramic block set




Order No.

Accuracy	Steel	Ceramic	Description
Grade 0	516-111-10	516-116-10	16-piece set with 12mm and 25mm thick optical parallels and Arkansas grinding stone
Grade 1	516-112-10	516-162-10	
Grade 2	516-113-10	516-163-10	
Grade 0	516-103-10	516-152-10	10-piece set
Grade 1	516-101-10	516-153-10	
Grade 2	—	516-154-10	
Grade K	516-977-60	—	10-piece set with 12mm thick optical parallel
Grade 0	516-978-10	516-378-10	
Grade 1	516-979-10	516-379-10	
Grade 2	516-980-10	516-380-10	
Grade 0	516-106-10	516-156-10	10-piece set with 12mm thick optical parallel
Grade 1	516-107-10	516-157-10	
Grade 2	516-108-10	516-158-10	
Grade K	—	516-164-60	8-piece set
Grade 0	516-115-10	516-165-10	
Grade 1	516-116-10	516-166-10	
Grade 2	516-117-10	516-167-10	

Optical Flats

These Optical Flats are used for inspecting the flatness of micrometer's or gauge block's measuring faces with high accuracy.

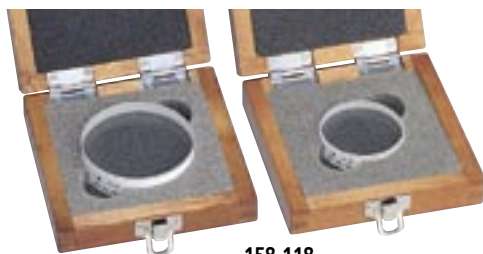

158-118

Specifications

Flatness	Order No.	Diameter	Thickness
0.1μm	158-118	45mm	12mm
0.1μm	158-120	60mm	15mm
0.2μm	158-117	45mm	12mm
0.2μm	158-119	60mm	15mm

Micrometer Standards

These micrometer standards are used for the zero point setting of outside micrometers (over 25mm).

- Flatness of measuring faces: 0.3μm
- Parallelism between measuring faces: 2μm
- Standards for screw thread micrometer and V-anvil micrometer are also available.



Specifications

Order No.	Length	Tolerance	Diameter
167-101	25mm	±1.5μm	6.35mm
167-102	50mm	±2.0μm	6.35mm
167-103	75mm	±2.5μm	6.35mm
167-104	100mm	±3.0μm	7.9mm
167-105	125mm	±3.5μm	7.9mm
167-106	150mm	±4.0μm	7.9mm
167-107	175mm	±4.5μm	7.9mm
167-108	200mm	±5.0μm	9.4mm
167-109	225mm	±5.5μm	9.4mm
167-110	250mm	±6.0μm	9.4mm
167-111	275mm	±6.5μm	9.4mm
167-112	300mm*	±7.0μm	9.4mm

*Available up to 1000mm

Optical Parallels

These Optical Parallels are designed to inspect parallelism and flatness of measuring faces of micrometers. Each set comprises 4 thicknesses, enabling the parallelism to be checked at every 1/4 rotation of the spindle.



157-903

Specifications

Parallelism	Order No.	Flatness	Thickness	Diameter
0.2μm	157-903	0.2μm	12.00mm 12.12mm 12.25mm 12.37mm	30mm
0.2μm	157-904	0.2μm	25.00mm 25.12mm 25.25mm 25.37mm	30mm

Inside Micrometer Calibration

CERA Inside Micro-Checker

- 10mm gauge blocks are arranged at 25mm intervals to efficiently check the zero point of a tubular inside micrometer.
- This checker can be used to calibrate inside micrometers if attachment holders and gauge blocks are arranged in appropriate lengths.
- For more information, refer to our General Catalog No.

Specifications

Range	Order No.	Accuracy
300mm	515-585	$\pm(1+L/150)\mu\text{m}$
600mm	515-586	L=Length to check (mm)



Depth Micrometer Calibration

Depth Micro-Checker

- The Depth Micro-Checker is designed to efficiently check the zero point of a depth micrometer.
- This checker can be used to calibrate depth micrometers if gauge blocks are arranged in appropriate lengths.
- For more information, refer to Mitutoyo's General Catalog.

Specifications

Range	Order No.	Accuracy
150mm	515-570	$\pm(1+L/150)\mu\text{m}$
300mm	515-571	L=Length to check (mm)




Calipers/Height Gage Calibration

CERA Caliper Checker

- For calibration of the vernier, dial and digital calipers as well as height gages in vertical position.
- For more information, refer to Mitutoyo's General Catalog.

Specifications

Range	Order No.	Block pitch accuracy	Parallelism of blocks
300mm	515-555	$\pm 5\mu\text{m}$ for range up to 300mm	$\pm 2\mu\text{m}$ for range up to 300mm
600mm	515-556	$\pm 7\mu\text{m}$ for range up to 600mm	$\pm 4\mu\text{m}$ for range up to 600mm

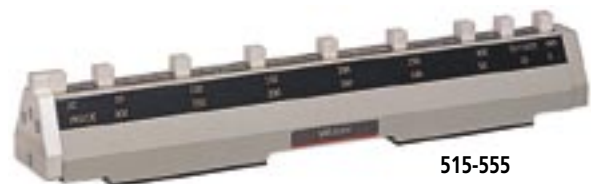

CMM/Machine Tool Calibration

Check Masters

- The Check Master is designed to check the accuracy of table movements of machine tools and calibrate CMMs.
- This master gage can be used in either vertical and horizontal orientation.
- Straight arrangement of 10mm block stack provides a calibration means at an interval of 20mm.

Specifications

Range	Order No.	Block pitch accuracy	Parallelism of blocks
300mm	515-720		
450mm	515-721	Up to 300mm: $\pm 2.5\mu\text{m}$	Up to 300mm: $1.2\mu\text{m}$
600mm	515-722	300 - 600mm: $\pm 3.5\mu\text{m}$	300 - 600mm: $1.5\mu\text{m}$
1000mm	515-723	600 - 1000mm: $\pm 5.0\mu\text{m}$	600 - 1000mm: $2.0\mu\text{m}$
1500mm	515-724	1000 - 1500mm: $\pm 8.0\mu\text{m}$	1000 - 1500mm: $2.5\mu\text{m}$
300mm	515-740*		
450mm	515-741*	Up to 300mm: $\pm 1.2\mu\text{m}$	Up to 450mm: $1.0\mu\text{m}$
600mm	515-742*	300 - 600mm: $\pm 1.8\mu\text{m}$	450 - 1000mm: $1.5\mu\text{m}$
1000mm	515-743*	600 - 1000mm: $\pm 2.5\mu\text{m}$	1000 - 1500mm: $2.0\mu\text{m}$
1500mm	515-744*	1000 - 1500mm: $\pm 4.0\mu\text{m}$	

*Available with CERAMIC block stack at request.



CMM calibration with Check Master No. 515-742



Quadra-Square Master

Reference master for inspection of kinetic accuracy of machine tools, coordinate measuring machines and other precision measuring instruments where straightness or perpendicularity is critical.

- Finished with the heritage ultra precision lapping technique developed in gauge block manufacture, the four faces on the Quadra-Square Master can serve as reference.
- Straightness and perpendicularity of four faces are finished with closer tolerance of $1\mu\text{m}/300\text{mm}$ or less. Perpendicularity of the reference face to the side face is within $5\mu\text{m}$.



Specifications

Order No.	Dimensions (WxLxT)	Reference Faces perpendicularity/flatness	Side Faces perpendicularity/parallelism
311-101	80x100x25mm	$1\mu\text{m}/1\mu\text{m}$	$5\mu\text{m}/5\mu\text{m}$
311-102	160x200x25mm	$1\mu\text{m}/1\mu\text{m}$	$5\mu\text{m}/5\mu\text{m}$
311-103	250x300x25mm	$1\mu\text{m}/1\mu\text{m}$	$5\mu\text{m}/5\mu\text{m}$

CERA Straight Master

This is a master gage used for the straightness inspection of each axis movement such as a CMM, machine tool, semiconductor related equipment and form measuring machine. An alminaceramic material is adopted to achieve the significant weight reduction compared with the conventional masters made from a stone or iron. The CERA Straight Master is high precision, high rigidity and easy to carry.

- Alminaceramic made
- 50mm / 100" pitch gradation scales
- Precision lapped measuring surface
- Little secular change
- Lightweight



Specifications

Code No.	311-302	311-322	311-305	311-325	311-307	311-327	311-309	311-329
Nominal length	400mm	16"	700mm	28"	1000mm	40"	1300mm	50"
Section form	35x50mm/1.38"x1.97"				45mmx 80mm/1.78"x3.15"			
Straightness	$0.3\mu\text{m}$	$12\mu\text{in}$	$0.5\mu\text{m}$	$20\mu\text{in}$	$1\mu\text{m}$	$40\mu\text{in}$	$1.5\mu\text{m}$	$60\mu\text{in}$
Mass	1.8kg/3.96lb		3kg/6.6lb		8kg/17.6lb		10kg/22lb	

Mitutoyo

Dial Indicator/Dial Test Indicator/Bore Gage Calibration

Calibration Tester (170, 521 Series)

- 170 series dial gage tester is designed to calibrate measuring accuracy of 0.01mm reading gages; dial indicators (1mm, 5mm, 10mm and 20mm range), dial test indicators and bore gages.
- 521 series calibration tester is specially designed to calibrate measuring accuracy of 0.001mm reading gages; dial indicators (1mm and 5mm range) and dial test indicators. The model 521-103 is also available for calibration of electronic micrometers.
- For more information, refer to Mitutoyo's General Catalog.

Specifications

Order No.	Graduation	Range	Accuracy
170-102	0.001mm	0 - 25mm	±2.0µm
521-103	0.0001mm	0 - 1mm	±0.2µm
521-105	0.0001mm	0 - 5mm	±0.8µm



521-103



170-102

i-Checker

- Mitutoyo brings you $\pm(0.2+L/100)\mu\text{m}^{*1}$ indication accuracy - the world's highest - for higher inspection reliability with various types of indicators and probes.
- *¹ When inspecting in vertical posture.
- Now you can directly inspect an indicator with a stroke of up to 100mm. What's more, optional accessories let you inspect the dial test indicator, bore gage and lever-type inductive head each with a different form of support.
- Adjustment of the measurement position is very easily accomplished because of semi-automatic measurement and full automatic measurement functions.
- It is possible to create own simple inspection certificate.
- It is possible to save inspection result as CSV file for reusable inspection result by any kind of software.
- For more information, refer to Catalog No. E4217 "i-Checker".



i-Checker main unit

Item	Contents
Measuring Range	100mm/4"
Resolution	0.02µm/8µin
Accuracy (at 20°C)	vertical position $\pm(0.2+L/100)\mu\text{m}$ L = Arbitrary length lateral position $\pm(0.3+2L/100)\mu\text{m}$ L = Arbitrary length
Feed speed	4mm/sec (max.)
Drive method	Motor drive
Measuring Unit	Reflective-type metal linear encoder
Thermal expansion coefficient of measurement mode	$(8\pm 1)\times 10^{-6}/\text{K}$
Measurement method	Semiautomatic measurement Fully automatic measurement Digimatic Indicator with RS-232C output
Input data connector	Digimatic data input connector X1 Flat cable connector 10pin/equivalent to XG4-1301 from OMRON
Dimensions (W x D x H)	184x225x532mm/7.24"x8.86"x20.94"
Operating temperature range	20°C ±3°C
Operating humidity range	58%RH±15%RH (Only free of condensation)
Storage temperature range	-10°C to 50°C
Storage humidity range	5%RH to 90%RH (Only free of condensation)
Power supply	100VAC to 240VAC ±10%, 50/60Hz
Mass	20kg/44.1lbs

Order No.

	Bush supplied	User's Manual	Calibration certificate
170-302■	ø8	A4 size	—
170-303■	ø3/8"	A4 size	—
170-304■	ø8	8.5"x11" size	—
170-305■	ø3/8"	8.5"x11" size	—
170-302■-01	ø8	A4 size	Supplied
170-303■-01	ø3/8"	A4 size	Supplied
170-304■-01	ø8	8.5"x11" size	Supplied
170-305■-01	ø3/8"	8.5"x11" size	Supplied

Note: To denote your AC line voltage fill the blank of order number with the following suffixes (e.g. 170-302A). A for 120V, D for 220V, E for 240/220V. No suffix is required for 100V.

Profile Projector/Measuring Microscope Calibration

Standard Scale and Reading Scale for profile projectors (172 Series)

- The Standard Scales are used for checking magnification accuracy of the profile projectors and microscopes.
- The Reading Scales are specially designed for inspecting the magnified image of a standard scale on the projection screen.

Specifications (Standard Scale)


Graduation	Range	Order No.	Accuracy (L=Length to check (mm))
0.1mm	50mm	172-116	$\pm(3+5L/1000)\mu\text{m}$
0.1mm	80mm	172-330	$\pm(3+5L/1000)\mu\text{m}$

Specifications (Reading Scale)

Graduation	Range	Order No.	Accuracy (L=Length to check (mm))
0.5mm	200mm	172-118	$\pm(15+15L/1000)\mu\text{m}$
0.5mm	300mm	172-161	$\pm(15+15L/1000)\mu\text{m}$
0.5mm	600mm	172-329	$\pm(15+15L/1000)\mu\text{m}$

Standard Scale (182 Series)

- High precision line standard manufactured under Mitutoyo's leading-edge Linear Scale production technology.
- High accuracy is guaranteed to be used as a standard for calibrating graduated scales.
- Made of low expansion glass.
- Coefficient of thermal expansion: $0.08 \times 10^{-6}/\text{K}$


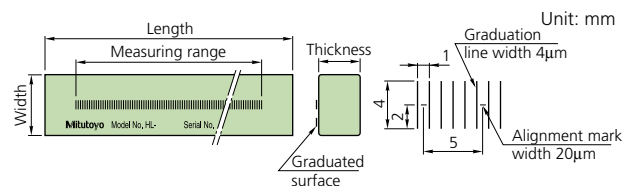


Specifications

Range	Order No.	Graduation		Accuracy (at 20°C)	Dimensions		
		Pitch	Thickness		Length	Width	Thickness
250mm	182-501	1mm	4µm	0.75µm	280mm	20mm	10mm
500mm	182-502	1mm	4µm	1µm	530mm	30mm	20mm

Working Standard Scale (182 Series)

- High precision line standard manufactured under Mitutoyo's leading-edge Linear Scale production technology.
- Ideal for checking the table feeding accuracy of measuring equipment and the semiconductor production equipment.
- Made of sodium glass.
- Coefficient of thermal expansion: $(8 \pm 1) \times 10^{-6}/\text{K}$

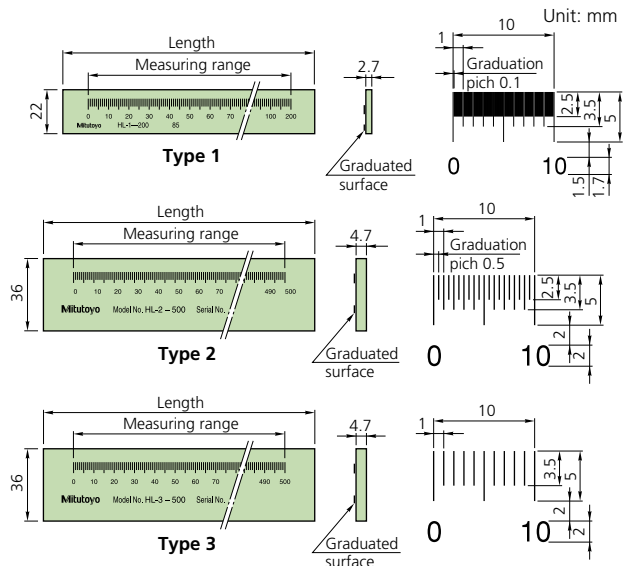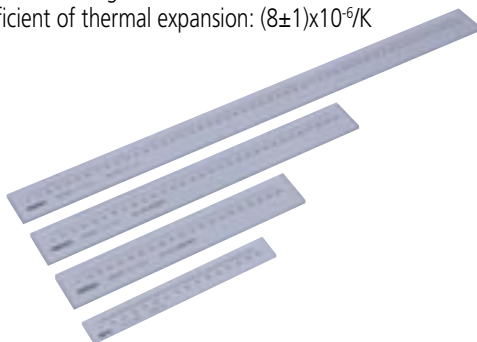

Specifications

Range	Order No.	Graduation		Accuracy (at 20°C)	Length	Type
		Pitch	Thickness			
50mm	182-511	0.1mm	20µm	1.6µm	75mm	Type 1
100mm	182-512	0.1mm	20µm	1.7µm	125mm	Type 1
150mm	182-513	0.1mm	20µm	1.8µm	175mm	Type 1
200mm	182-514	0.1mm	20µm	1.9µm	225mm	Type 1
100mm	182-521	0.5mm	50µm	1.7µm	130mm	Type 2
200mm	182-522	0.5mm	50µm	1.9µm	230mm	Type 2
300mm	182-523	0.5mm	50µm	2.1µm	330mm	Type 2
400mm	182-524	0.5mm	50µm	2.3µm	430mm	Type 2
500mm	182-525	0.5mm	50µm	2.5µm	530mm	Type 2
250mm	182-531	1mm	100µm	2.0µm	280mm	Type 3
500mm	182-532	1mm	100µm	2.5µm	530mm	Type 3
750mm	182-533	1mm	100µm	3.0µm	780mm	Type 3
1000mm	182-534	1mm	100µm	3.5µm	1030mm	Type 3

Snap Gage (C-gage) Calibration

Snap Gage Checker

The Snap Gage Checker is capable of inspecting the snap gage of sizes up to 320mm quickly and accurately with resolution down to 0.0001mm.



Specifications

Order No.	515-611K (110V) 515-611A (120V) 515-611D (220V) 515-611E (240V)
Resolution	0.0001mm
Range	20 - 320mm
Block travel	100mm
Block pitch accuracy	±0.001mm
Parallelism of blocks	0.001mm
Block feeding error	±0.002mm
Measuring force	4 - 10N (available)

Height Measurement Standard/Surface Plate

Height Masters

- The Height Master is used as a reference gage of the height measurement.
- This master gage features the staggered arrangement of block stack which has two measuring faces on the same level, one facing up and the other facing down.
- Riser blocks (blocks for increasing the height) are also available.
- For more information, refer to Mitutoyo's General Catalog.



Specifications

Range	Order No.	Resolution	Description
5 - 310mm	515-322	0.001mm	Standard type
10 - 310mm	515-354	0.001mm	Digital type
10 - 460mm	515-356	0.001mm	Digital type
10 - 610mm	515-358	0.001mm	Digital type
5 - 310mm	515-341	0.0001mm	Digital type (100V)
5 - 310mm	515-341A	0.0001mm	Digital type (120V)
5 - 310mm	515-341D	0.0001mm	Digital type (220V)
5 - 310mm	515-341E	0.0001mm	Digital type (240V)

		515-322	515-354 515-356	515-358	515-341
Block pitch accuracy	Up to 300mm:	±1.5µm	±1.5µm	±1.5µm	±0.5µm
	300 - 450mm		±2.5µm	±2.5µm	
	450 - 600mm			±3.5µm	
Parallelism of blocks	Up to 300mm:	1.0µm	2.0µm	2.0µm	0.5µm
	300 - 600mm		2.5µm	2.5µm	
Block feeding error		±1.0µm	±2.0µm	±2.5µm	±0.5µm



Graplate (Granite Surface Plate)


This is used for a reference surface plate in the height and perpendicularity measurements and layout work.

Specifications

Dimensions (W x D x Hmm)	Order No.			Flatness (mm)			Steel stands (optional)		
	00 grade	0 grade	1 grade	00 grade	0 grade	1 grade	Order No.	h (adjustable)	Remark
300 x 300 x 100	517-401-4	517-301-4	517-101-4	0.002	0.003	0.005	—	—	—
450 x 300 x 100	517-411-4	517-311-4	517-111-4	0.002	0.003	0.006	—	—	—
600 x 450 x 100	517-414-4	517-314-4	517-114-4	0.0025	0.004	0.008	517-203/203R*/203CR**	755 - 780mm	With levelling bolt
600 x 600 x 130	517-403-4	517-303-4	517-103-4	0.0025	0.005	0.008	517-204/204R*/204CR**	785 - 810mm	With levelling bolt
750 x 500 x 130	517-405-4	517-305-4	517-105-4	0.003	0.005	0.009	517-205/205R*/205CR**	785 - 810mm	With levelling bolt
1000 x 750 x 150	517-407-4	517-307-4	517-107-4	0.003	0.007	0.012	517-206/206R*/206CR**	755 - 780mm	With levelling bolt
1000 x 1000 x 150	517-409-4	517-309-4	517-109-4	0.0035	0.008	0.013	517-207/207R*/207CR**	735 - 775mm	With levelling bolt
1500 x 1000 x 200	517-413-4	517-313-4	517-113-4	0.004	0.008	0.016	517-208/208R*/208CR**	735 - 775mm	With levelling bolt
2000 x 1000 x 250	517-410-4	517-310-4	517-110-4	0.0045	0.010	0.019	517-209/209R*/209CR**	735 - 775mm	With levelling bolt
2000 x 1500 x 300	517-416-4	517-316-4	517-116-4	0.005	0.010	0.020	517-210/210R*/210CR**	735 - 775mm	With levelling bolt
2000 x 2000 x 300	517-417-4	517-317-4	517-117-4	0.0055	0.011	0.022	O6AAY174	700 - 706mm	—
3000 x 1500 x 400	517-418-4	517-318-4	517-118-4	0.0065	0.013	0.025	O6AAY175	700 - 706mm	—
3000 x 2000 x 500	517-419-4	517-319-4	517-119-4	0.007	0.014	0.027	O6AAY176	700 - 706mm	—

*with drop prevention device
**with caster wheel

Calibration Standards/Instruments and Accredited Calibration Services

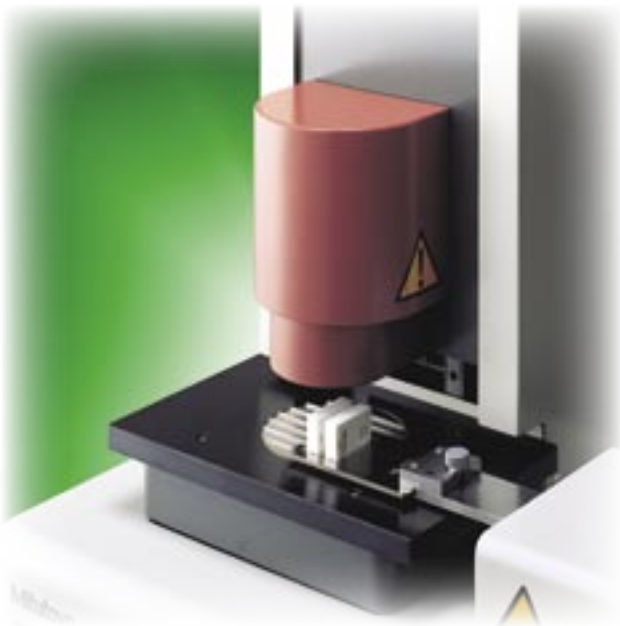

Specifications are subject to change without notice.

Note: All information regarding our products, and in particular the illustrations, drawings, dimensional and performance data contained in this pamphlet, as well as other technical data are to be regarded as approximate average values. We therefore reserve the right to make changes to the corresponding designs, dimensions and weights. The stated standards, similar technical regulations, descriptions and illustrations of the products were valid at the time of printing. In addition, the latest applicable version of our General Trading Conditions will apply. Only quotations submitted by ourselves may be regarded as definitive.

Coordinate Measuring Machines

Vision Measuring Systems

Surface-, Form- and Contour Measurement

Optical Measuring

Sensor Systems

Hardness Measuring

Digital Scale and DRO Systems

Small Tool Instruments and Data Management

Mitutoyo Corporation

20-1, Sakado 1-Chome,
Takatsu-ku, Kawasaki-shi,
Kanagawa 213-8533, Japan
Phone (044) 813-8230
Fax (044) 813-8231
<http://www.mitutoyo.co.jp>

Mitutoyo